

JPD-100S (mini)



AngelSounds®

Fetal Doppler

INSTRUCTION MANUAL

Manual Version: V1.1
Issuing Date: 2020.11

Product Information

Product Name: Fetal Doppler

Model: JPD-100S (mini)

Manufacturer: Shenzhen Jumper Medical Equipment Co., Ltd

Address: D Building, No. 71, Xintian Road, Fuyong Street,
Baoan, Shenzhen, Guangdong, China

Copyright

Copyright 2016. All rights reserved.

Statement

Shenzhen Jumper Medical Equipment Co., Ltd owns the copyright of this non-public instruction book.

Without authorization from Shenzhen Jumper Medical Equipment Co., Ltd, any individual or organization shall not copy, modify or translate this book.

All contents described in this book are consistent with the actual situation of the related product.

Shenzhen Jumper Medical Equipment Co., Ltd has right to revise all contents of this book if needed, without prior notice.

Shenzhen Jumper Medical Equipment Co., Ltd reserves the right of final interpretation of this book.

"ANGELSOUNDS" is the registered trademark of Shenzhen Jumper Medical Equipment Co., Ltd.



Please read the User Manual carefully to make sure safe and proper use of this Fetal Doppler, Please read and fully understand the Safety Precautions before use.

Precaution Labels Definition

The signal words shown below, left, identify the potential hazard categories. The definition of each category is as follows:



DANGER: This alert identifies hazards that will cause serious personal injury or death.



WARNING: This alert identifies hazards that may cause serious personal injury or death.



CAUTION: This alert identifies hazards that may cause minor personal injury, product damage, or property damage.

NOTE: The label indicates what you should attention.

Table of contents

SECTION 1: INSTRUCTION.....	1
1.1 CONTACT INFORMATION.....	1
1.2 INDICATION FOR USE.....	2
1.3 PRODUCT DESCRIPTION.....	2
1.4 OPERATING PRINCIPLE.....	2
1.5 CONTRAINDICATIONS FOR USE.....	3
1.6 ADVERSE EFFECTS.....	3
SECTION 2: SAFETY GUIDANCE.....	3
2.1 SAFETY ALERT DESCRIPTIONS.....	3
2.2 SYMBOLS.....	5
SECTION 3: GETTING STARTED.....	7
3.1 UNPACKING AND INSPECTING.....	7
SECTION 4: CONTROLS AND INDICATORS.....	8
4.1 APPEARANCE.....	8
4.2 INDICATOR.....	8
4.3 KNOB.....	8
4.4 SOCKET.....	8
4.5 BATTERY.....	9
SECTION 5: OPERATION PROCEDURE.....	9
5.1 PREPARATION.....	9
5.2 DETECTING.....	10
5.3 RECORDING.....	11
SECTION 6 PREVENTIVE MAINTENANCE.....	11
6.1 MAINTENANCE.....	11
6.2 VISUAL INSPECTION.....	12
6.3 CLEANING PRODUCT AND ACCESSORIES.....	13
6.4 DISINFECTIONS.....	15
6.5 RECYCLE BATTERIES.....	15
6.6 AUTHORIZED REPAIR SERVICE.....	15
SECTION 7: TECHNICAL SPECIFICATIONS.....	15
SECTION 8 : TROUBLESHOOTING.....	17
APPENDIX A EMC INFORMATION.....	18

Section 1: Instruction

Become familiar with the controls and how to use the product properly before operating the product.



CAUTION: Federal law restricts this device to be sold by or on the order of a physician or practitioner licensed by state law in which he/she practices to use or order the use of the device.



CAUTION: It should not be used in life supporting or life sustaining applications



CAUTION: It cannot replace the professional fetal monitor, when the fetal heart rate is abnormal, or can not find the fetal heart, can not feel the fetal movement, pregnant woman's should immediately go to the hospital to seek the doctor's help.

Intended use

The Fetal Doppler JPD-100S(mini) is a hand-held, battery powered audio Doppler device used for detecting fetal heartbeats.

1.1 Contact Information

Manufacturer: Shenzhen Jumper Medical Equipment Co., Limited;
Manufacturer Address: D Building, No. 71, Xintian Road, Fuyong Street, Baoan, Shenzhen, Guangdong, China
Tel.: +86-755-26696279
Fax: +86-755-26852025
E-mail: info@jumper-medical.com
Website: <http://www.jumper-medical.com>

Manufacturing:



Shenzhen Jumper Medical Equipment Co., Limited;
Address: D Building, No. 71, Xintian Road, Fuyong Street, Baoan, Shenzhen, Guangdong, China

Authorized European Representative:



MedPath GmbH
Mies-van-der-Rohe-Strasse 8, 80807 Munich, Germany

1.2 Indication for Use

This device can detect the Fetal Heart Rate. Connect the headset allows for hearing the sound of the fetal heartbeat. You can count the fetal heart rate when listening. This device normally is applied to 16 weeks gestation or later, difference in pregnant mater.

The device detects fetal life from early gestation thru delivery, and it can be a general indication of fetal well being.

The normal range of fetal heart rate: 110bpm-160bpm.

1.3 Product Description

The product is a lightweight, portable detector. It is designed to meet your detecting and hearing needs by providing advanced detecting functions and a full range of sound of the fetal heartbeat.

The product is mainly used to detect the fetal heartbeat rate (FHR) and the sound of the fetal heartbeat (SFH).

The growth and development of a fetus can be found out through examination of these indices. It is applicable for department of gynaecology and obstetrics and clinic daily.

In accordance with classification criteria in Annex IX on "Medical Device Directive 93/42/EEC", the product is class IIa based on rule 10, "Devices for Direct Diagnosis or Detection on physiological process".

The Product is powered by a 9V internal battery.

1.4 Operating Principle

Fetal Doppler consists of transmitter unit, receiver unit, signal process unit, and signal output unit (such as headset).

Ultrasonic wave is transmitted from one piezoelectric ceramic at the front of the probe to the uterus of the pregnant women. Echo is received by the other piezoelectric ceramic at the front of the probe when ultrasonic wave reaches the fatal heart. Then it is converted into voltage. This doppler signal is detected and demodulated from the received signal. And the Doppler frequency is consistent with the rhythm of the

fetal systole and diastole. Once cardiac valves vibrate and a Doppler frequency excursion is formed. It is transmitted an output signal of cardiac valves vibrating, and it is sent to signal demodulate unit to get the Doppler frequency signal, and process the signal become the signal that can be heard by human using headset.

1.5 Contraindications for Use

Normally none, as a particular case, please consult your doctor.

1.6 Adverse effects

No adverse effect.

1.7 USE Note for use

This device cannot replace a professional fetal monitor. If the fetal heart rate is abnormal or cannot be located using this monitor, immediately go to the hospital to seek the doctor's help. If fetal movement is not felt by the pregnant woman, immediately go to the hospital to seek the doctor's help.

Section 2: Safety Guidance

This product is internal powered equipment, and the degree of shock protection is B applied part.



It means that these person connections will comply with permitted leakage currents, dielectric strengths of IEC/EN60601.

2.1 Safety alert descriptions

The following is a list of product safety alerts that appear in this section and throughout this manual. You must read, understand, and heed these safety alerts before attempting to operate the Product.



DANGER: Fire and Explosion Hazard

Do not operate the product in the presence of flammable gases to avoid possible explosion or fire hazard.



WARNING: Use only Approved Equipments

Do not use batteries, gel, cables, or optional equipment other than those approved by Jumper Medical Ultrasonic Instrument Co., Ltd. which may cause the Product to function improperly during a rescue.



WARNING: Adjacent and/or Stacked Equipment

The product should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, the product should be observed to verify normal operation in the configuration in which it will be used.



WARNING: Practice the ALARA principle

We recommend that exposure to ultrasound should be kept as low as reasonably achievable principle. This is considered to be good practice and should be observed at all time.



WARNING: Aid healthcare professional tool

The product should not be used in place of normal fetal monitoring. It is a tool to aid the healthcare professional.



CAUTION: Temperature/Humidity/Pressure Extremes

Exposing the Product to extreme environmental conditions outside of its operating parameters may compromise the ability of the Product to function properly.



CAUTION: Battery Disposal

Recycle or dispose of the battery in accordance with all federal, state and local laws. To avoid fire and explosion hazard, do not burn or incinerate the battery.



CAUTION: Possible Radio Frequency (RF) Susceptibility

RF susceptibility from cellular phones, CB radios and FM 2-way radio may cause interference with the Product. Do not operate wireless radiotelephones in the vicinity of the Product – turn power OFF to the radiotelephone and other like equipment near the Product.



CAUTION: Systems Statement

Equipment connected to the Product must be certified to the respective IEC Standards (i.e. IEC 60950 for data processing equipment and IEC 60601-1 for medical

equipment). Furthermore, all configurations shall comply with the system standard IEC 60601-1-1. Anybody who connects additional equipment to the signal input part or signal output part configures a medical system, and is therefore, responsible that the system complies with the requirements of the system standard IEC 60601-1-1. The Product Service Port is only intended for use during maintenance by authorized service personnel.



CAUTION: Case Cleaning Solutions

When disinfecting the case, use a non-oxidizing disinfectant, such as ammonium salts or a glutaraldehyde based cleaning solution, to avoid damage to the metal connectors.



CAUTION: Environment of use

The Product is designed for indoor use. Operator must confirm that the environment of use meets the required operating environmental specifications before using.



CAUTION: Cold Environments

If the Product is stored in an environment with a temperature below the operating temperature, the unit should be allowed to warm up to the needed operating temperature before using.

















CAUTION: Product recycling or disposal

The product could be sent back to the manufacturer for recycling or proper disposal after their useful lives.

2.2 Symbols

The following symbols may appear in this manual, on the Product, or on its accessories. Some of the symbols represent standards and compliances associated with the Product and its use.

	Consult instructions for use of the Product and/or its accessories.
	Warning Information

	Authorized Representative in the European Community
	CE Mark: The Product system conforms to essential requirements of the Medical Device Directive 93/42/EEC.
	Date of manufacture.
	Manufacturer information
	Storage Temperature limit
	Humidity limitation
	Atmospheric Pressure limitation
	Upward
	Specifies serial number of the Product
	LOT Number
	It indicates that the equipment should be sent to the special agencies according to local regulation for separate collection after its useful life.
	Type B applied part
IPX4	Ingress Protection.

Section 3: Getting Started

This section presents information on unpacking the Product.

This section contains a list of parts for product. To place an order, contact your representative or distributor.

3.1 Unpacking an Inspecting

Every attempt is made to ensure your order is accurate and complete. However, to be sure that your order is correct, verify the contents of the box against your packing slip.

The product is designed for simplicity of operation and set-up and requires minimal assembly. The following item is packing list:

No.	Item	Quantity	Packed or Unpacked
1	Instruction Manual	1	√
2	Product	1	√
3	Recording Cable	1	√
4	Headset	1	√
5	Battery	1	√

Carefully inspect each item as it is unpacked for any signs of damage which may have occurred during shipment.


- Check the components according to the packing list.
- Check for any damage or defects. Do not attempt to setup the Product if anything is damaged or defective. Contact Jumper Medical Equipment Co., Limited Ultrasonic Instrument Customer Service immediately if anything is damaged or defective.

Section 4: Controls and indicators

This section provides the basic set up information. You need to read this section in detail before operating the device.

4.1 Appearance

1. Power On/Off / Volume knob
2. Power indicator
3. Headset Socket
4. Transducer
5. Battery Compartment Cover
6. Audio output socket

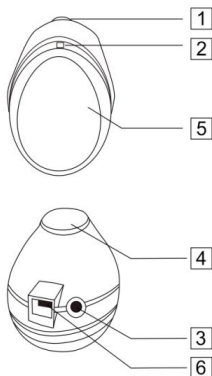

4.2 Indicator

There is an indicating light on JPD-100S(mini).

2. Power indicator

Function: Power on indicate.

4.3 Knob

There is a knob on JPD-100S(mini).

Power on/off and volume knob

1. Power On/Off / Volume knob

Function: Power on or off the device, change the volume of the speaker.

4.4 Socket

There are one headset socket and one USB interface used as audio out socket at the device.

3. Headset Socket 6. Audio output socket

The headset socket can be connected with headset.

The USB interface is used to connect recording Cable (**NOTE:** please refer to accessories).

4.5 Battery

This device is internal powered. The power of JPD-100S (mini) comes from a 9V alkaline battery (IEC type No. 6F22 or equivalent).

Section 5: Operation procedure


This section provides the description for operation.

5.1 Preparation

Follow these recommendations to preparation for operation:

5.1.1 Install Battery

Open the battery cover, and install the 9V battery. Then, Install the battery cover.

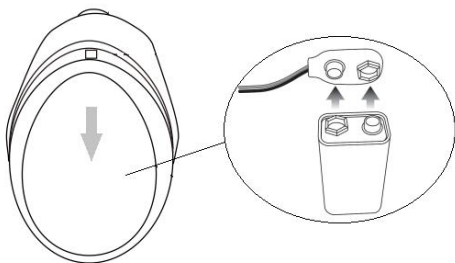

NOTE : You should push the battery cover backward like the figure upward.

Then you can open the battery cover.

Battery type: Alkaline battery 9V



CAUTION:

Remove the battery if the device is not likely to be used for some time. And keep the battery in cool and dry environment.



WARNING: Irregular treatment of batteries may be result in hazards to health and environment.

5.1.2 Connect headset

Before you practice the product, you should prepare an earphone or a headset to hear the fetal heartbeat sound.

We will give you a headset as a present. It can help you to hear the fetal heartbeat sound when you have not bought an earphone.

Insert the headset-plug into headset socket, and wire the handset.

5.1.3 Power on by turning the Power on/off and volume knob

1. Power On/Off / Volume knob


5.1.4 Remove clothes from the pregnant maternal abdomen.

5.1.5 Applying couple gel to the faceplate (**4. Transducer**) of probe or abdomen of pregnant woman.

5.2 Detecting

5.2.1 Find the fetal heart and listen the fetal heartbeat sound

Locate the position of the fetus by hand touching, firstly to find out the best direction to the fetal heart. The position of the fetal heart in abdomen of pregnant woman you can contrast the figure below. Place the faceplate of probe at the best position for detecting fetal heartbeat. Adjust the transducer to obtain an optimum audio signal ideally by angling the transducer around. Generally, the site of heart of fetus is 1/3 below of navel line at its earlier stage, it then moves upward with increasing of gestational period, and the site of heart of fetus will be a little deviation to left or right with different fetus. Please make sure that the surface of the probe should be contacted fully with the skin. After the sound become clear, it is the proper functioning. If no coupling gel, water can be used.

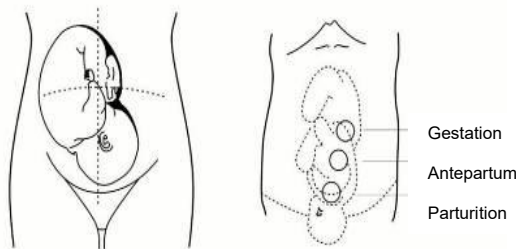

5.2.2 Calculate the fetal heart rate

Count the fetal heartbeat sound in one minute, the number you counted is the fetal heartbeat rate. Repeat count at least 3 times, you will get the range of fetal heartbeat rate.

5.3 Recording

When you hear the fetal heartbeat sound, you can connect one socket with a headset, and another can connect with computer. You can replay the recorded sound files anytime, and you can send them whoever you want.

Section 6 Preventive maintenance

Proper maintenance of the product is very simple, yet it is an important factor of its reliability. The section describes the maintenance and service required for the product and its accessories.

6.1 Maintenance

WARNING: Failure on the part of all responsible individuals, hospitals or institutions, employing the use of Product, to implement the recommended maintenance schedule may cause equipment failure and possible health hazards. The manufacturer does not, in any manner, assume the responsibility for performing the recommended maintenance

schedule. The sole responsibility rests with the individuals, hospitals, or institutions utilizing the product.

1. The transducer acoustic surface is frangible and must be handled with care. Gel must be wiped off from the transducer after use. These precautions will prolong the life of the unit.
The user must check that the equipment does not have visible evidence of damage that may affect patient safety or product's capability before use. The recommended inspection interval is once per month or less. If damage is evident, replacement is recommended before use.
2. To ensure the product is always functional when required, the following maintenance shall be performed:
 - Visual Inspection
 - Cleaning the product and its accessories
 - Check the battery fuel gauge
 - Testing product Performance

Correction: manually calculate the FHR with hearing fetal heartbeat sound for qualification.

Recommended maintenance and care:

- It is important that the Product is stored at the operating temperature range if it is expected to be used. Optimal battery life will be obtained if stored and operated at room temperature. See Section 7 for Temperature Specifications.
- The Product requires no calibration.

6.2 Visual Inspection

The product and its accessories should be carefully inspected prior to installation, once every 16 months thereafter and each time the equipment is serviced.

- Carefully inspect the equipment for physical damage
- Inspect all external connections for loose connectors or frayed cables.

- Verify that the Safety label on back of the product is clearly legible

INSTRUCTION	INSPECT FOR	RECOMMENDED REMEDY
Examine the case connectors and accessories	Foreign substances	Clean the Product and its accessories as described.
	Damage or cracks	Contact Our Customer Service
Examine accessory cables	Foreign substances	Clean the cables as described in the Section 5
	Broken parts, cracks, damage, or extreme wear, broken or bent connectors and pins, after bending and flexing the cable	Replace cable if any abnormalities are found.
Examine disposable accessories	Expired product or Product pads	Replace any products approaching or past their expiration dates.



WARNING: After the visual inspection, if the Product and/or its accessories are damaged please contact our Customer Service. The Product will need to be returned back to us for repair. The accessories should be disposed of appropriately and replacement parts shall be ordered.

6.3 Cleaning Product and Accessories

Listed below are recommendations for cleaning the Product and its accessories.

Recommended cleaning product:

The following cleaning products may be used to clean the exterior surfaces of the Product as well as the batteries.

- Do not use abrasive cleaners or strong solvents such as acetone or acetone-based cleaners.

- Do not mix disinfecting solutions (such as bleach and ammonia) as hazardous gases may result.
- Do not clean electrical contacts or connectors with bleach.

Cleaning instructions:

1. Before cleaning the Product, turn off the device and disconnect the power cord.
2. Before cleaning, remove all adherent soil (tissue, fluids, etc.) and wipe thoroughly with a cloth dampened with water before applying the cleaning solution.
3. When cleaning, do not immerse. Keep the exterior surface of the device clean and free of dust and dirt, clean exterior surface of the unit with a dry, soft cloth .if necessary, clean it with a soft cloth soaked in a solution of soap and wipe dry with a clean cloth immediately. Wipe the transducer body with soft cloth to remove any remaining coupling gel .Clean with soap only
4. Wring any excess moisture from the cloth before cleaning.
5. Avoid pouring fluids on the device, and do not allow fluids to penetrate the exterior surfaces of the device.
6. To prevent scratching the display, the use of a soft cloth is recommended.



CAUTION: To prevent damage to equipment, do not clean any part of the Product or Accessories with phenolic compounds. Do not use abrasive or flammable cleaning agents. Do not steam, autoclave, or gas-sterilize the Product or accessories.



CAUTION: Cleaning liquids: Do not submerge the device in liquids or pour cleaning liquids over, into or onto the device.

- * Don't use strong solvent, for example, acetone.
- * Never use an abrasive such as steel wool or metal polish.
- * Do not allow any liquid to enter the product, and do not immerse any parts of the device into and liquids.
- * Avoid pouring liquids on the device while cleaning.

* Don't remain any cleaning solution on the surface of the device.
Wipe the surface of sensor of transducer with 70% ethanol or alcohol, self-air dry or clean with a clean, dry cloth.

6.4 Disinfections

Cleaning the unit surface and the transducer as the above mentioned, then wipe the surface of transducer with 70% ethanol or alcohol, clean the transducer surface with a dry, soft cloth.

- * Don't use low temperature steam sterilization or other way to sterilize
- * Don't use high temperature sterilizing process

6.5 Recycle Batteries

The battery is recyclable. Remove the old battery from the Product and follow your local recycling guidelines or Refer to local regulations.



WARNING: Irregular treatment of batteries may be result in hazards to health and environment.

6.6 Authorized Repair Service

The Product has no user-serviceable internal components. Try to resolve any maintenance issues with the Product by using the Troubleshooting Table presented in this chapter. If you are unable to resolve the problem, contact Jumper Medical Equipment Co., Limited Service.

NOTE: The warranty will be void upon unauthorized disassembly or service of the product.

Section 7: Technical specifications

This section presents the specifications and safety standards of the product.

NOTE: The following specifications are subject to change and are only noted as a point of reference.

Product name: Fetal Doppler

Mode: JPD-100S(mini)

Safety: Complies with IEC 60601-1, EN 60601-1, EN60601-1-2, IEC 61266

Classification:

Anti-electric shock type: Internal powered equipment

Anti-electric shock degree: Type B applied part.



Classification of protection against harmful ingress of water:

Ordinary protection IPX4(probe)

Methods of sterilization or disinfection: No sterilization required the equipment

Degree of Safety in Presence of Flammable Gases: Equipment not suitable for use in the presence of flammable gases

Mode of operation: Continuous operation

EMC: Group I Class B

Technical parameters:

Ultrasound:

Ultrasonic emitting frequency: 3MHz

Overall sensitivity at the distances 200mm from the face of the probe
(Doppler frequency: $500 \pm 50\text{Hz}$, Target velocity: $10\text{cm/s} \sim 40\text{cm/s}$): $\geq 90\text{dB}$

Spatial-peak temporal-peak acoustic pressure: $\leq 1\text{MPa}$

Output power: $< 20\text{mW}$

Effective area of the ultrasonic transducer active element: $2.65\text{cm}^2 \pm 0.3\text{cm}^2$

The acoustic coupling medium for normal use: ph: $5.5 \sim 8$, Acoustic impedance: $\leq 1.7 \times 10^5\text{g/cm}^2 \cdot \text{s}$

Working mode: Continuous wave Doppler

Audio output:

Audio output power: $< 0.5\text{ W}$

Audio out Socket: $\Phi 3.5\text{mm}$ /USB interface

Recommended battery type:

9V DC alkaline battery (IEC Type No. 6F22 or equivalent)

Stand-by Time: $> 4\text{hours}$

Suitable gestation: 16 gestational weeks or later, difference in pregnant mater.

Physical Characteristic:

Size: 104.5mm(length) * 50mm(width) * 70mm(height)

Weight: 69.5g (only main unit, not including battery)

Environmental Requirements:

Operating Conditions:

Temperature: 5°C to 40°C

Humidity: 0 to 80% RH, non-condensing

Atmospheric pressure: 86kPa to 106kPa

Storage and Shipping Conditions:

Temperature: -20°C to 55°C (-4°F -131°F)

Humidity: 10 to 93% RH, non-condensing

Atmospheric pressure: 50kPa to 106kPa

Section 8 : Troubleshooting

What appearance to be a malfunction may not always serious, if your product should not perform as expected, consult the table below to see if the problems can be corrected before seeking help from your dealer or service representative.

Symptom	Cause	Remedy
Audio scream	<ul style="list-style-type: none">● Audio volume too high● Too much gel on the probe surface● Battery is exhausted	<ul style="list-style-type: none">● Turn down the volume● Use less gel● Replace the batteries
Weak sound output	<ul style="list-style-type: none">● Audio volume too low● Insufficient gel● Battery is exhausted	<ul style="list-style-type: none">● Turn up the volume● Add gel● Replace the battery

Low sensitivity	<ul style="list-style-type: none"> ● Incorrect probe position ● Insufficient gel 	<ul style="list-style-type: none"> ● Locate the correct position ● Add gel
-----------------	--	--

Appendix A EMC Information



CAUTION:

Fetal Doppler needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided for in the ACCOMPANYING DOCUMENTS.



CAUTION:

Portable and mobile RF communications equipment can affect **Fetal Doppler**.



CAUTION:

The **Fetal Doppler** should not be used adjacent to or stacked with other equipment.

A1.1 Electromagnetic Emissions


The Fetal Doppler is intended for use in the electromagnetic environment specified below. The customer or the user of the Fetal heart monitor should assure that it is used in such an environment.		
Emissions	test	Compliance
RF emissions CISPR 11	Group 1	The Fetal Doppler uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	The Fetal Doppler is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.

A 1.2 Electromagnetic Immunity

The Fetal Doppler is intended for use in the electromagnetic environment specified below. The customer or the user of the Fetal Doppler should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±6 kV contact ±8 kV air	±6 kV contact ±8 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30 %.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	3 A/m	3 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

A 1.3 Electromagnetic Immunity (not life-supporting)

The Fetal Doppler is intended for use in the electromagnetic environment specified below. The customer or the user of the Fetal Doppler should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2,5 GHz	3 V/m	Portable and mobile RF communications equipment should be used no closer to any part of the Fetal Doppler including cables, than the recommended

		<p>separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance</p> $d = 1,2\sqrt{P}$ $d = 1,2\sqrt{P} \quad 80 \text{ MHz to } 800 \text{ MHz}$ $d = 2,3\sqrt{P} \quad 800 \text{ MHz to } 2,5 \text{ GHz}$ <p>a. Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in metres (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, should be less than the compliance level in each frequency range.</p> <p>b. Interference may occur in the vicinity of equipment marked with the following symbol:</p> 
<p>NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies.</p> <p>NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.</p>		
<p>a. Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Fetal Doppler is used exceeds the applicable RF compliance level above, the</p>		

Fetal Doppler should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the **Fetal Doppler**.
 b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

1.4 Recommended Separation Distances

Recommended separation distances between portable and mobile RF communications equipment and the **Fetal Doppler**.

The **Fetal Doppler** is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the **Fetal Doppler** can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the **Fetal Doppler** as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter (m)		
	150 kHz to 80 MHz $d = 1,2\sqrt{P}$	80 MHz to 800 MHz $d = 1,2\sqrt{P}$	800 MHz to 2.5 GHz $d = 2,3\sqrt{P}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations.

Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

AngelSounds®



Shenzhen Jumper Medical Equipment Co., Ltd.
Address: D Building, No. 71, Xintian Road, Fuyong Street,
Baoan, Shenzhen, Guangdong, China
Tel.: +86-755-26696279 Fax.: +86-755-26852025
Website: <http://www.jumper-medical.com>